




PUSEN

Single Use Grasping & Biopsy Forceps

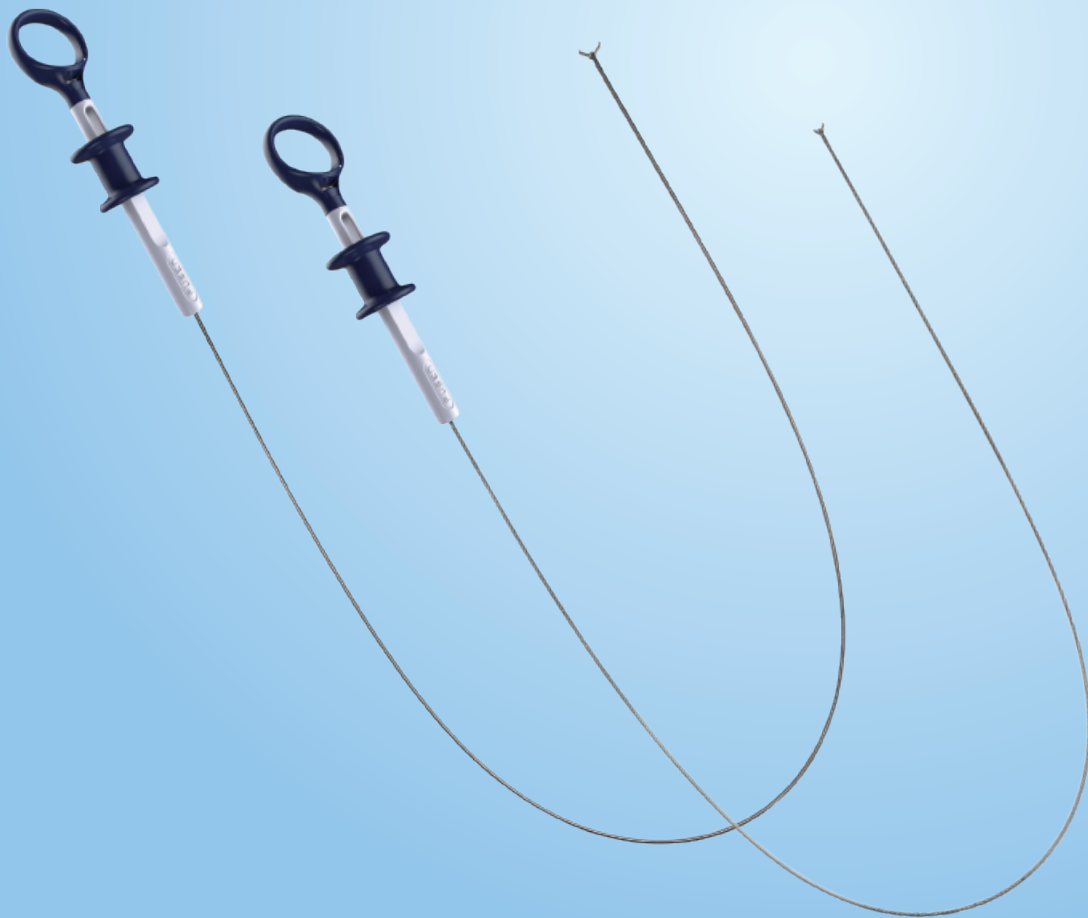

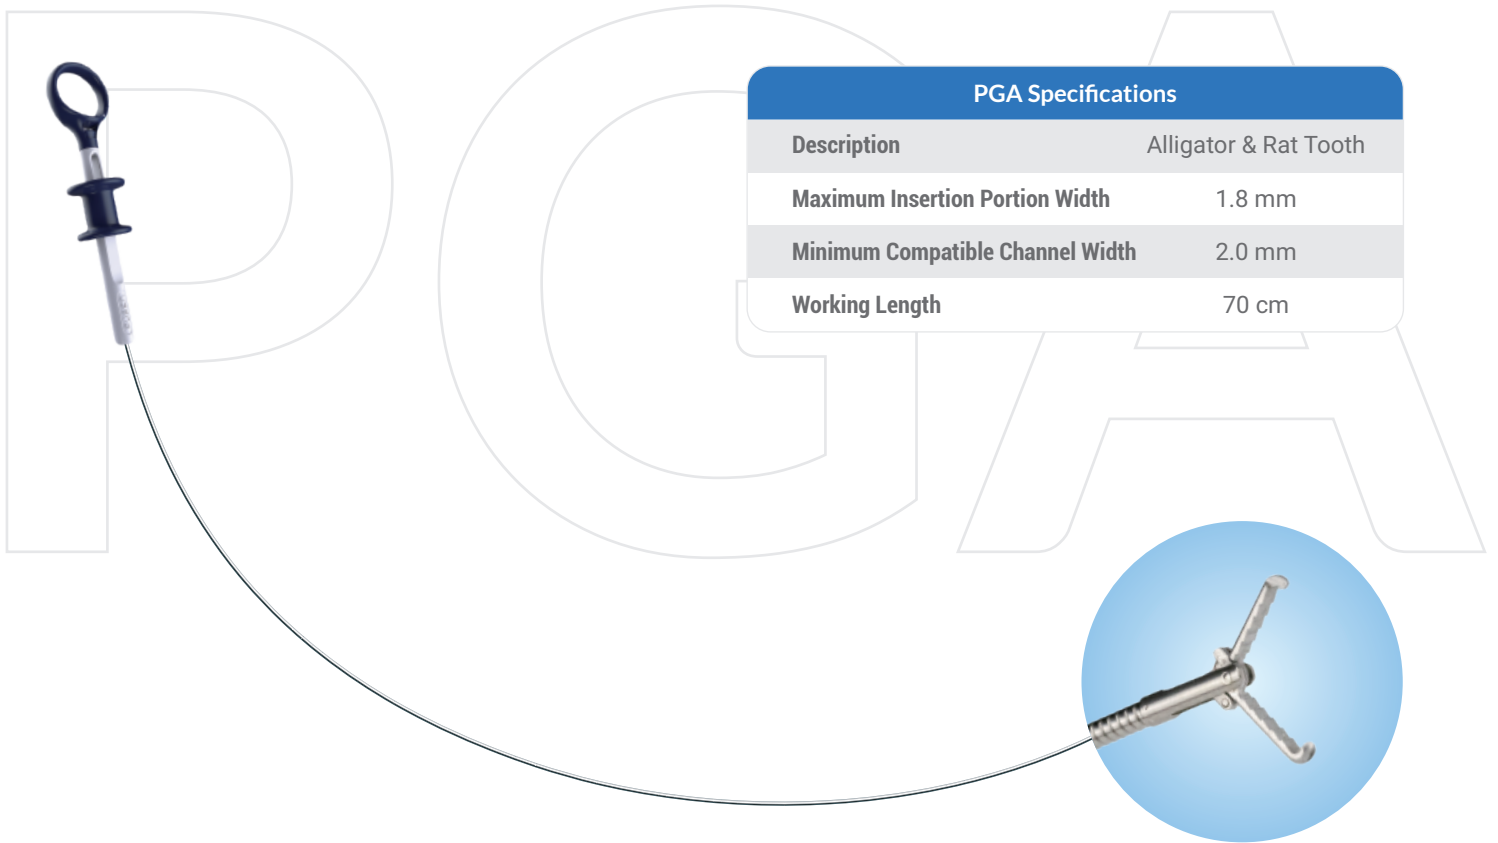

PGA Specifications	
Description	Alligator & Rat Tooth
Maximum Insertion Portion Width	1.8 mm
Minimum Compatible Channel Width	2.0 mm
Working Length	70 cm

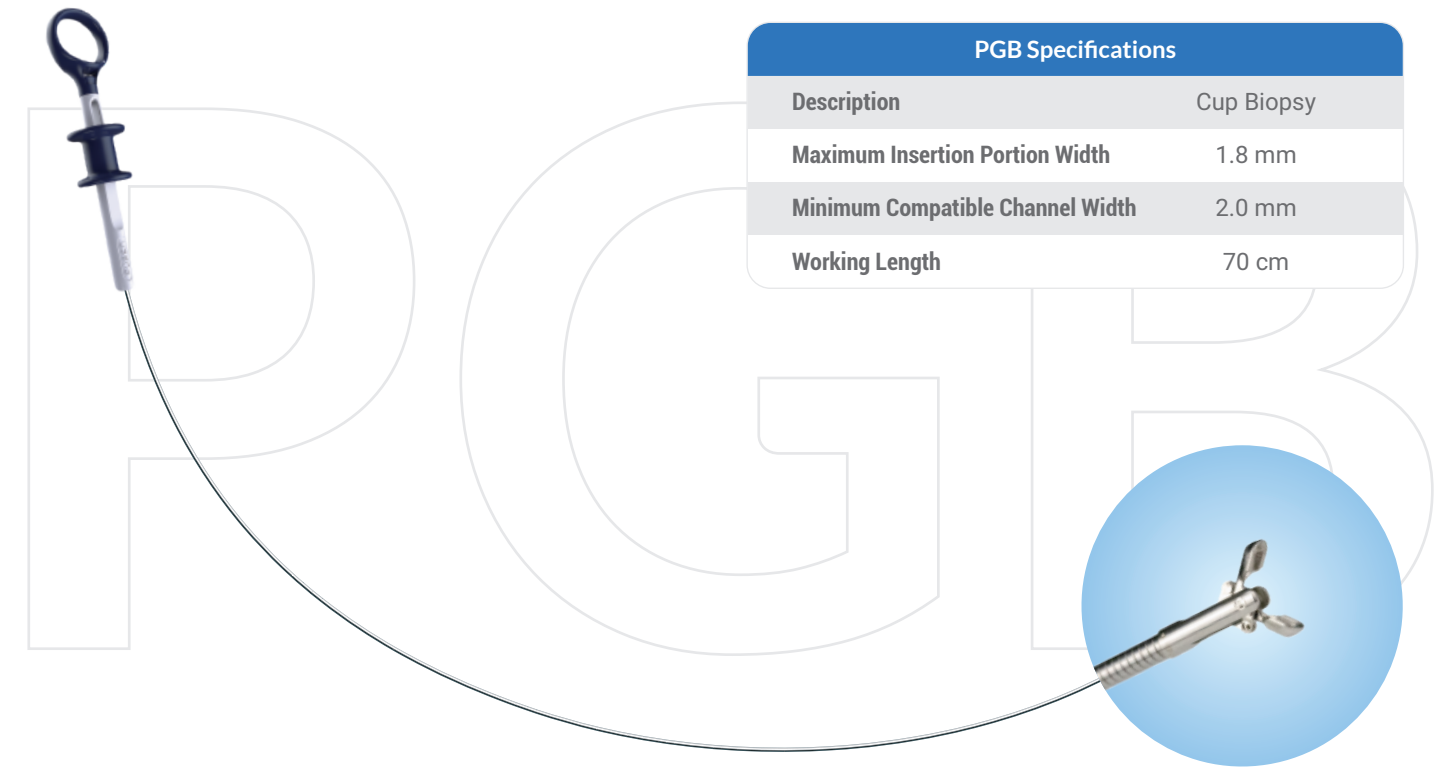

PGB Specifications	
Description	Cup Biopsy
Maximum Insertion Portion Width	1.8 mm
Minimum Compatible Channel Width	2.0 mm
Working Length	70 cm

PUSEN

PUSEN USA Inc

11340 Lakefield Dr, STE 200

Johns Creek, GA, 30097

989-467-8736

(989)-GO-PUSEN

info@PUSENUA.com

Ver-US-202507